

Physician: Sample Report  
 Patient: Sex:  
 Accession #: 2017000000  
 Collected:

Age:  
 Sample Type: Serum  
 Received:


Date of Birth:  
 Completed:

IgA   
 IgG 


CLIA #: 50D0965661  
 COLA accredited

**Dairy**

*Bovine-derived unless specified*

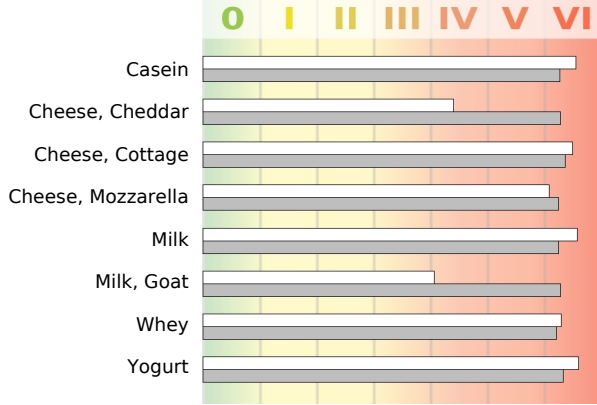


**Grains/Legumes/Nuts**

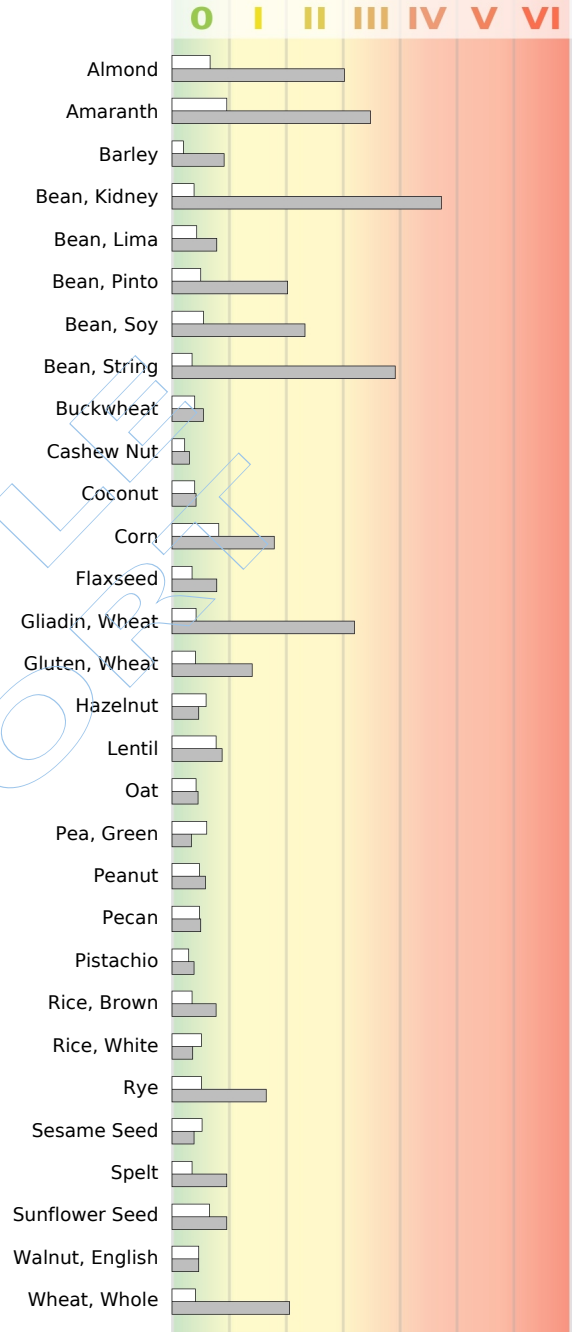

**Egg**



**Misc**

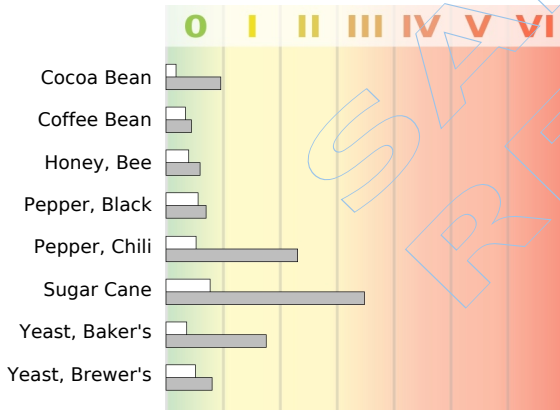

US BioTek Laboratories' proprietary ELISA analyses are designed to assay specific total IgG (subclasses 1, 2, 3, 4), total IgA (subclasses 1, 2), and IgE antibodies. The classification of 0 to VI denotes the level of IgG, IgA, and/or IgE antibodies detected through spectrophotometric analysis. The antigens on the panel are subject to change without prior notice. Reference ranges are updated periodically.

This test was developed and its performance characteristics determined by US BioTek Laboratories, Inc. It has not been cleared or approved by the U.S. Food and Drug Administration.

Physician: Sample Report  
 Patient: Sex:  
 Accession #: 2017000000  
 Collected:

Age:  
 Sample Type: Serum  
 Received: Completed:



Date of Birth:

IgA   
 IgG

CLIA #: 50D0965661  
 COLA accredited

**Vegetables**

**Fruits**

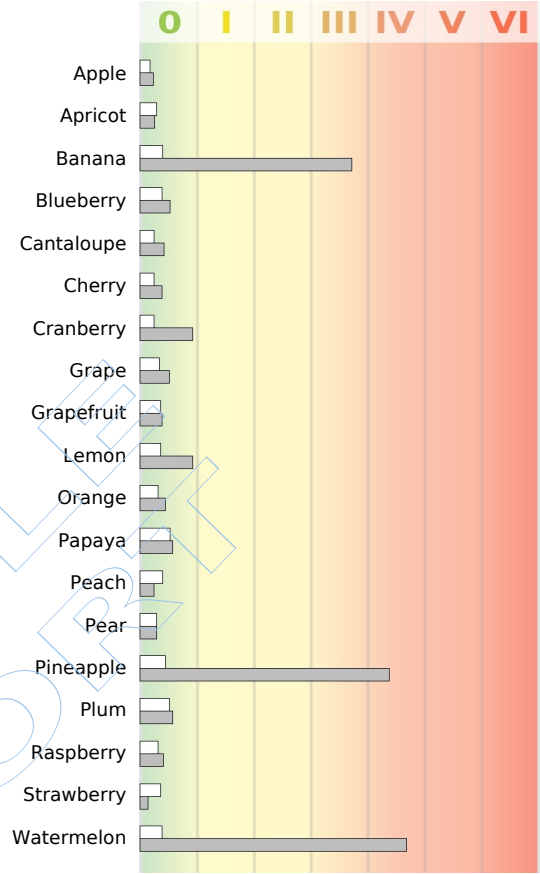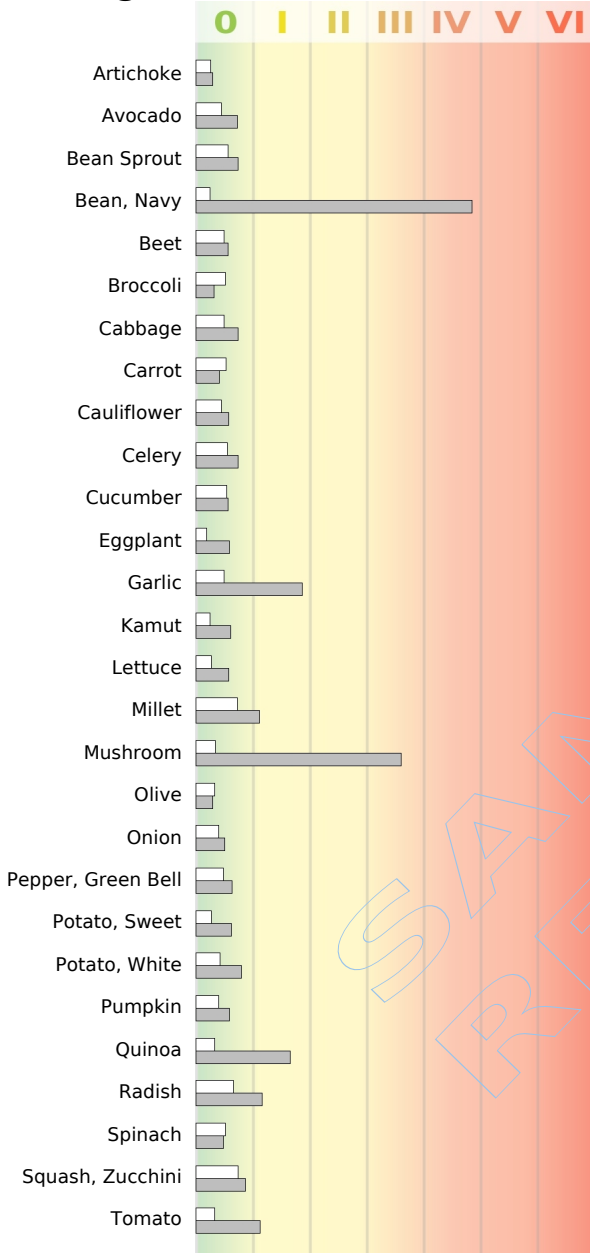

© US BioTek Laboratories

Reaction Class

Director: Stephen Markus, MD



US BioTek Laboratories' proprietary ELISA analyses are designed to assay specific total IgG (subclasses 1, 2, 3, 4), total IgA (subclasses 1, 2), and IgE antibodies. The classification of 0 to VI denotes the level of IgG, IgA, and/or IgE antibodies detected through spectrophotometric analysis. The antigens on the panel are subject to change without prior notice. Reference ranges are updated periodically.

This test was developed and its performance characteristics determined by US BioTek Laboratories, Inc. It has not been cleared or approved by the U.S. Food and Drug Administration.